



Improving the accuracy of multi breath-hold diffusion tensor MRI tractography of the heart using dynamic motioncorrection

Citation

Mekkaoui, Choukri, Sonia Nielles-Vallespin, Marcel P Jackowski, Peter D Gatehouse, Dudley J Pennell, David N Firmin, and David E Sosnovik. 2013. Improving the accuracy of multi breath-hold diffusion tensor mri tractography of the heart using dynamic motioncorrection. Journal of Cardiovascular Magnetic Resonance 15(Suppl 1): 081.

Published Version

doi:10.1186/1532-429X-15-S1-081

Permanent link

<http://nrs.harvard.edu/urn-3:HUL.InstRepos:11235650>

Terms of Use

This article was downloaded from Harvard University's DASH repository, and is made available under the terms and conditions applicable to Other Posted Material, as set forth at <http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA>

Share Your Story

The Harvard community has made this article openly available.
Please share how this access benefits you. [Submit a story](#).

[Accessibility](#)



ORAL PRESENTATION

Open Access

Improving the accuracy of multi breath-hold diffusion tensor MRI tractography of the heart using dynamic motion correction

Choukri Mekkaoui*, Sonia Nielles-Vallespin, Marcel P Jackowski, Peter D Gatehouse, Dudley J Pennell, David N Firmin, David E Sosnovik

From 16th Annual SCMR Scientific Sessions
San Francisco, CA, USA. 31 January - 3 February 2013

Background

Diffusion Tensor MRI (DTI) tractography of the human heart can be performed *in vivo*, but requires multiple breatholds per slice to achieve adequate SNR [1,2]. The physiological noise inherent to multiple breatholds results in a diffusion-encoded volume in which the data vary as a function of space and time. This may hinder the assessment of diffusion based-indices in the heart and accurate tractography of myofiber architecture. In this study, we investigate the effect of a novel automated motion correction method on *in vivo* DTI of the heart.

Methods

DTI of 10 normal volunteers was performed on a 3T clinical scanner (Skyra, Siemens) with the following parameters: 6 diffusion-encoding directions, $b=350 \text{ s/mm}^2$, fat saturation, TR/TE=1100/23 ms, BW=2442 Hz/pixel, spatial resolution=2.7x2.7x8 mm³, 8 averages. This required 24 separate breatholds for a 3-slice diffusion-encoded volume. On a chosen reference frame, n radial scanlines (Figure 1A) starting at the LV-RV junction and crossing at the center of the LV cavity were defined as the registration axes. Motion was estimated by matching the intensity gradient profiles of corresponding radial scanlines between frames and at all 3 slice levels. A rigid registration described by a set of translations and rotations was then determined between pairs of images, iteratively (Figure 1B). Convergence was achieved upon reaching a global minimum of the quadratic error at each level. The signal-noise-ratio (SNR) was calculated at each pixel \mathbf{r} with a given number of averages (repetitions) t , such that SNR_t

$(\mathbf{r}) = \text{MEAN}_t(\mathbf{r}) / \text{SD}_t(\mathbf{r})$ [3]. SNR, with and without motion correction, was measured in each voxel at end-diastole and end-systole. Fiber tracking was performed with a 4th order Runge-Kutta approach [4].

Results

At end-diastole, an increase of 24% was observed in the SNR of the T2-weighted images, and an average SNR increase of 21% was seen in the diffusion-weighted images (Figure 1C). At end-systole, a relatively uniform SNR increase of 15% was seen with motion correction for diffusion-free and diffusion-weighted images. Figure 2 shows tractograms in the lateral wall of the left ventricle at end-diastole and end-systole. Motion correction frequently increased the fiber track lengths, consistent with the observed increase in SNR, and in some cases also rectified their orientation (see endocardial fibers at end-systole, Figure 2B vs. 2D).



Conclusions

DTI tractography can be performed *in vivo* over multiple breatholds, but is affected by physiological noise. Here, we show that motion correction over space and time can reduce the noise produced by multiple breatholds while increasing the quality of the resulting tractograms. This approach paves the way for the use of free breathing navigator-based DTI for high-resolution tractography of the heart.

Funding

R01HL093038.

Radiology, Harvard Medical School - Massachusetts General Hospital, Boston, MA, USA

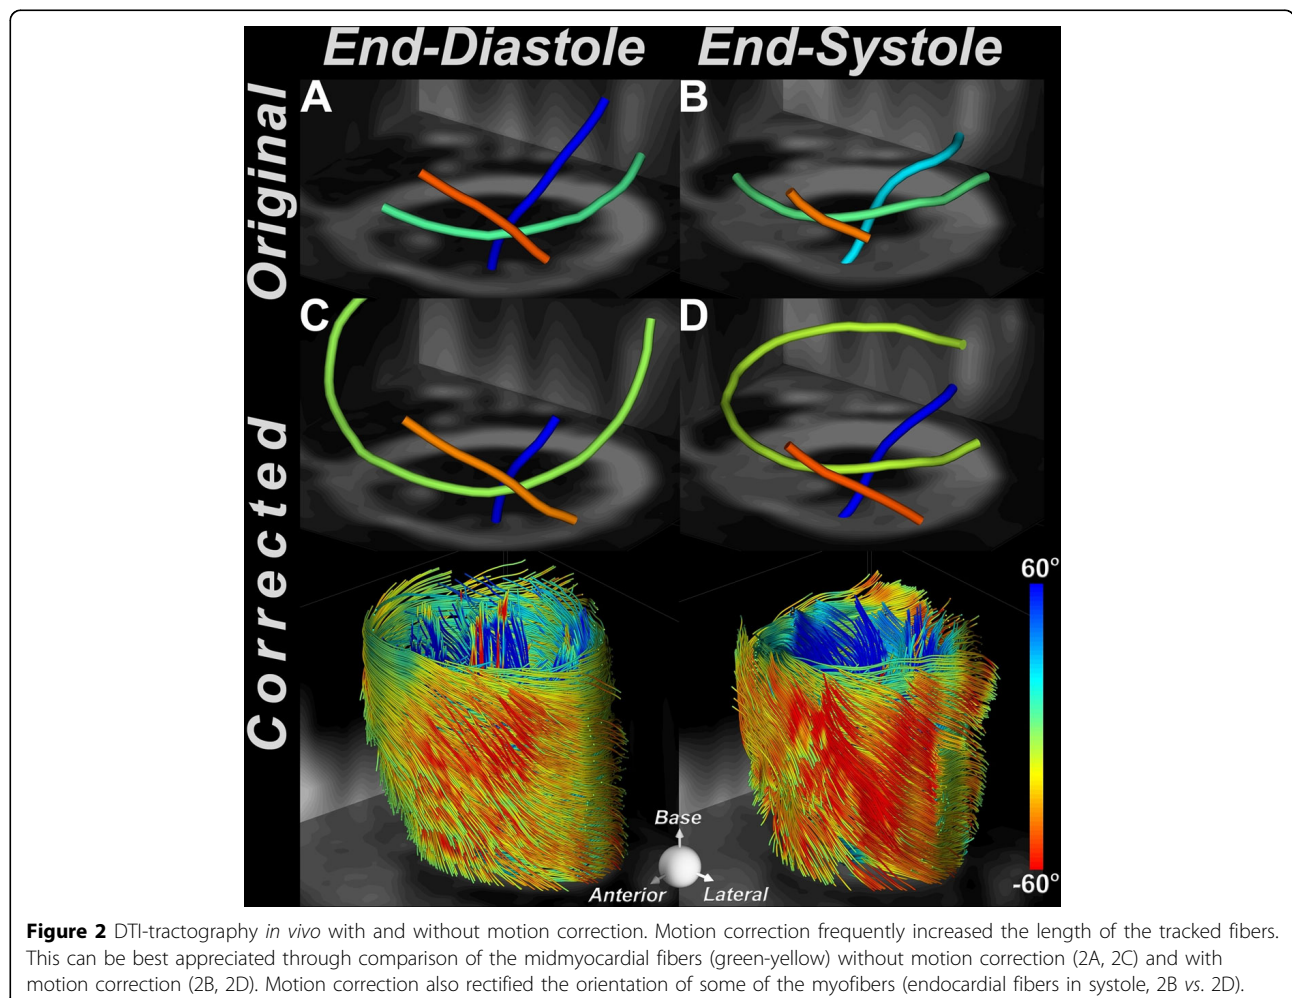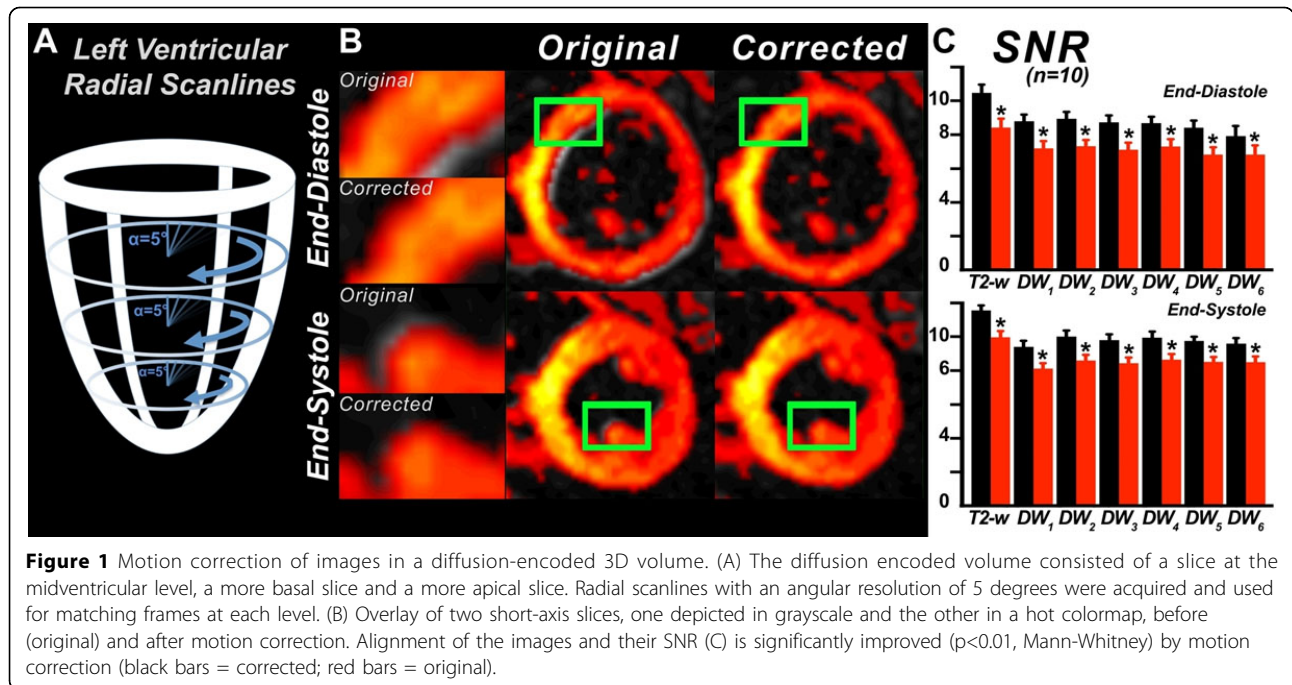

Published: 30 January 2013

References

1. Reese TG, et al.: *Magn Reson Med* 1995.
2. Nielles-Vallespin S, et al.: *Magn Reson Med* 2012.
3. Reeder SB, et al.: *Magn Reson Med* 2005.
4. Mekkaoui, et al.: *J Cardiovasc Magn Reson* 2012.

doi:10.1186/1532-429X-15-S1-O81

Cite this article as: Mekkaoui et al.: Improving the accuracy of multi breath-hold diffusion tensor MRI tractography of the heart using dynamic motion correction. *Journal of Cardiovascular Magnetic Resonance* 2013 15(Suppl 1):O81.

**Submit your next manuscript to BioMed Central
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

