



Accelerated three-dimensional free-breathing first pass cardiac perfusion at 1.5T

Citation

Akcakaya, Mehmet, Tamer A Basha, Murilo Foppa, Kraig V Kissinger, Warren J Manning, and Reza Nezafat. 2013. Accelerated three-dimensional free-breathing first pass cardiac perfusion at 1.5T. *Journal of Cardiovascular Magnetic Resonance* 15(Suppl 1): P42.

Published Version

doi:10.1186/1532-429X-15-S1-P42

Permanent link

<http://nrs.harvard.edu/urn-3:HUL.InstRepos:11181132>

Terms of Use

This article was downloaded from Harvard University's DASH repository, and is made available under the terms and conditions applicable to Other Posted Material, as set forth at <http://nrs.harvard.edu/urn-3:HUL.InstRepos:dash.current.terms-of-use#LAA>

Share Your Story

The Harvard community has made this article openly available.
Please share how this access benefits you. [Submit a story](#).

[Accessibility](#)



POSTER PRESENTATION

Open Access

Accelerated three-dimensional free-breathing first pass cardiac perfusion at 1.5T

Mehmet Akcakaya^{1*}, Tamer A Basha¹, Murilo Foppa¹, Kraig V Kissinger¹, Warren J Manning^{1,2}, Reza Nezafat¹

From 16th Annual SCMR Scientific Sessions
San Francisco, CA, USA. 31 January - 3 February 2013

Background

Perfusion CMR provides an important diagnostic tool for the detection of myocardial ischemia in patients with known or suspected CAD [1]. Conventionally, 2D multi-slice imaging with 2-4 short-axis slices is often used for evaluation of left ventricular perfusion. 3D CMR perfusion has been proposed for its superior coverage and higher SNR [2]. However, accelerated imaging is required for adequate spatio-temporal resolution. Recent studies in accelerated CMR have shown that utilizing local information in the imaging volume significantly improves reconstruction quality [3,4]. However, such highly accelerated k-t based techniques used for 3D perfusion [3] require breath-hold acquisitions, which may be difficult following physical stress or for some patients. In this study, we sought to develop a compressed-sensing (CS) based image reconstruction technique utilizing local imaging features for highly-accelerated 3D free-breathing perfusion CMR.

Methods

9 patients (46.0±14.8 years; 6 males) underwent 3D perfusion CMR on a 1.5T Philips Achieva magnet. Images were acquired using a saturation-recovery GRE sequence (TR/TE/α=2.1/1.2 ms/20°). 7.5-fold random undersampling, with fully-sampled central k-space (11 × 3 in ky-kz) was used to acquire 8 slices at 2.3 × 2.3 × 10 mm³ resolution within a 250 ms imaging window.

In the proposed reconstruction technique, each dynamic was first reconstructed individually with total variation

(TV) regularization, which were then used for utilizing local features as follows: 10×10 image patches were hypothesized to be slowly-varying across 5 consecutive heartbeats. The locality in each volume was used to capture how various anatomies move differently, whereas the locality in time was used to reduce temporal blurring artifacts due to free-breathing. Principal component (pc) bases were derived for each of these 10 × 10 × 1 × 5 overlapping image volumes. Then the distinct x-pc sparsity of these volumes was used for thresholding the image in an iterative B₁-weighted technique. Comparison images were generated using dynamic-by-dynamic (DBD) TV reconstruction, reconstruction using a pc basis for the whole volume (x-pc), and zerofilling of the data. Images were then scored by a blinded reader (1=poor, 4=excellent).

Results



Figure 1 and 2 show example dynamics after contrast arrival in two subjects. The proposed technique is able to provide images with clearly defined borders, without temporal blurring. Subjective image quality scores demonstrate that the proposed method is significantly better than the others (3.0±0.7 vs. 2.3±0.7 for x-pc, 1.7±0.5 for DBD, 1.0±0.0 for zerofilled).

Conclusions

The proposed framework allows for 7.5-fold accelerated free-breathing 3D perfusion reconstruction at 1.5T. Further clinical studies are needed to assess its diagnostic value in patients with suspected CAD.

¹Medicine, Beth Israel Deaconess Medical Center, Harvard Medical School, Boston, MA, USA

Full list of author information is available at the end of the article

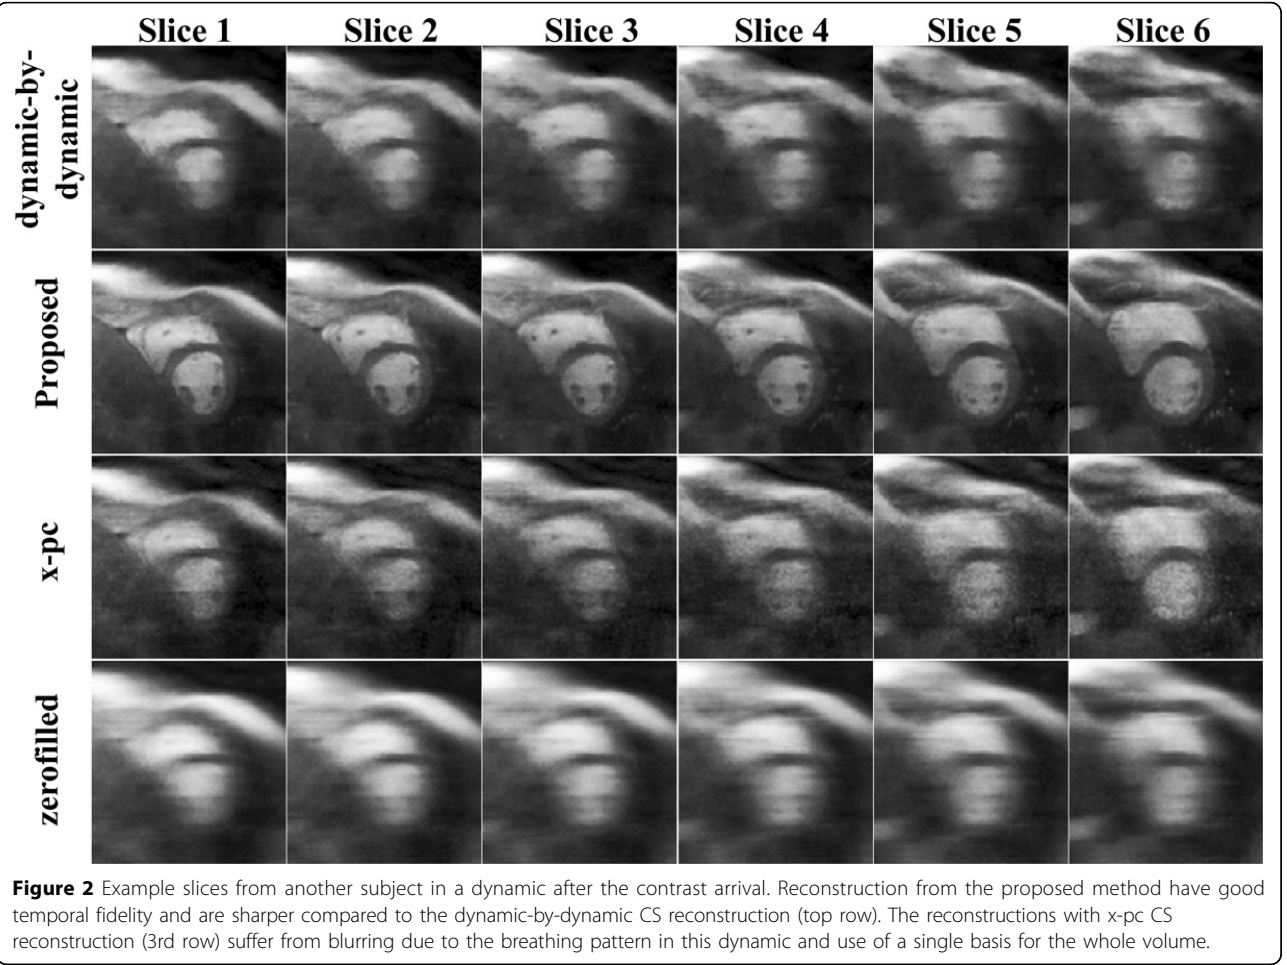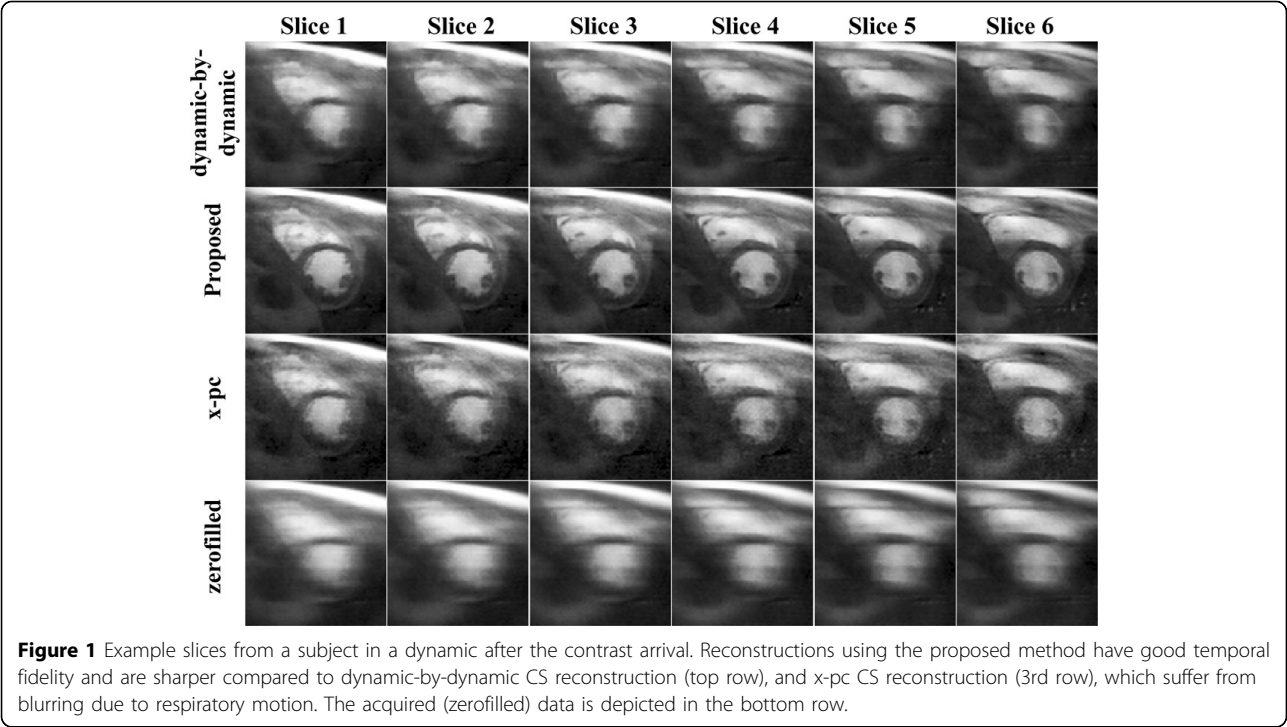

Funding

NIH:K99HL111410-01; R01EB008743-01A2.

Author details

¹Medicine, Beth Israel Deaconess Medical Center, Harvard Medical School, Boston, MA, USA. ²Radiology, Beth Israel Deaconess Medical Center, Harvard Medical School, Boston, MA, USA.

Published: 30 January 2013

References

1. Al-Saadi: *Circulation* 2000.
2. Shin: *JCMR* 2008.
3. Vitanis: *MRM* 2011.
4. Akçakaya: *MRM* 2011.

doi:10.1186/1532-429X-15-S1-P42

Cite this article as: Akcakaya et al.: Accelerated three-dimensional free-breathing first pass cardiac perfusion at 1.5T. *Journal of Cardiovascular Magnetic Resonance* 2013 **15**(Suppl 1):P42.

**Submit your next manuscript to BioMed Central
and take full advantage of:**

- Convenient online submission
- Thorough peer review
- No space constraints or color figure charges
- Immediate publication on acceptance
- Inclusion in PubMed, CAS, Scopus and Google Scholar
- Research which is freely available for redistribution

Submit your manuscript at
www.biomedcentral.com/submit

